





# Fast, Accurate, and Cost-effective

QUALITY - INNOVATION - FORESIGHT

For more information, go to tmi.yokogawa.com Test & Measurement Instruments

Bulletin AQ6150SR-01EN

1553.42

# **High performance and cost-effective Optical Wavelength Meter**

-16.48

-16.69

-13.12

-14.63


Exceeding the testing needs of optical devices and transmission systems

YOKOGAWA . ADSIS

1550.1161....

-8.50

The AQ6150 series optical wavelength meter is an ideal instrument for accurately measuring the optical wavelength of optical devices and systems used in telecommunication applications from 1270 to 1650 nm (Including C & L Band).

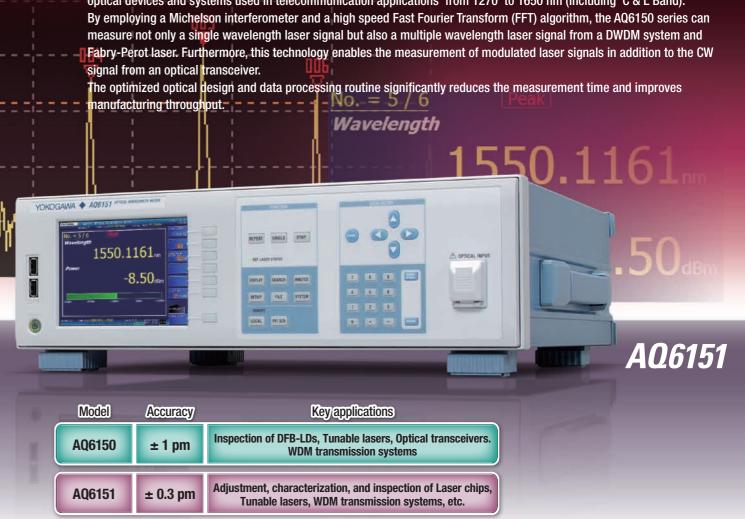

	Model	Accuracy	Keyapplications
X	AQ6150	±1pm	Inspection of DFB-LDs, Tunable lasers, O WDM transmission syste
	AQ6151	± 0.3 pm	Adjustment, characterization, and inspec Tunable lasers, WDM transmission

# Increase throughput with high speed measurement

For the adjustment and characterization of tunable laser sources and tunable optical transceivers requiring hundreds of wavelength measurements per device, high-speed measurement and processing capability are crucial for improving the production throughput.

Both models can acquire, analyze and transfer a measurement to a PC within



# **Reduce the lifetime ownership costs**

With the conventional wavelength meter, the high failure rate of the wavelength reference light source and its high replacement costs have been a major contribution to the overall ownership costs over the product life, not to mention disruptive downtime. One of the key product design goals was to address

these issues. We achieved this goal in a multi-dimensional approach as represented graphically on the right. First by extending the service life of the light source (Maximize Horizontal Scale). Second by reducing the replacement cost (Minimize Vertical Scale).

# Upgrade the test system with ease

Using a remote control interface, ETHERNET or GP-IB, you can easily build an automated measurement system. The remote command set complies with the commonly accepted SCPI industry standard command set for programmable

AQ6150 Series **Optical Wavelength Meter** 

# **Excellent wavelength measurement performance**

# High wavelength accuracy of $\pm 0.3$ pm

1546.7134

547.8463

AQ6150

There are two models in the series. The High Accuracy AQ6151 model offers an accuracy of  $\pm$  0.3pm to meet the most demanding precision requirements. The Standard Accuracy AQ6150 offers a  $\pm$  1pm accuracy for applications with less demanding requirements at a more affordable price. The real time correction feature utilizes a highly stable reference signal from the built-in wavelength reference light source in order to provide long-term stability for each and every measurement taken.

# Cope with modulated light and optical filter measurement

The optical output of optical transceivers and optical transmission systems is modulated with a transmission frequency like 10G and 40Gbps. The Built-In Optical Spectrum Analysis capability utilizing an FFT technique is required to measure the spectrum broadened by the modulated signal. In addition to the regular CW light mode, the AQ6150 Series has a modulated light mode. The modulated mode analyzes the optical spectrum and returns the center wavelength of the modulated light from the transceiver. This mode can also be used for the center wavelength measurement of optical filters such as a band pass filter, AWG and WSS.

# Simultaneous measurement of up to 1024 wavelengths

satur PLA Des

LOCAL PHY SID

0 0


Measure up to 1024 wavelengths in a single input signal with a minimum separation of 5GHz simultaneously, quickly, and accurately. This means it can meet testing needs in the development and production of WDM transmission system today and well into the future.

The multi-wavelength measurement capability contributes to production efficiency and cost reduction in the production of single wavelength laser devices as well by combining multiple laser modules or optical transceivers using an optical coupler and measuring all the signals at once.

# Maintain high performance even with low-power input

Equipped with an Auto Gain Control (AGC) function, the AQ6150 Series adjusts the gain of the electrical amplifier automatically based on the input signal power. This helps maximize wavelength accuracy and measurement speed even if the input signal power is as low as -40 dBm.

0.3 seconds! This is 5 times faster than our conventional model, thus vastly improving production throughput. In the Repeat measurement mode, the AQ6150 series can collect 5 measurements per second, making it extremely useful when adjusting a device while monitoring the wavelength in real time.



instruments. Thus, the existing measurement system can be easily upgraded without having to change the measurement program if Yokogawa AQ6140 series or another SCPI compatible optical wavelength meter is already in use.

# Various view modes

## • Single wavelength mode

The single wavelength mode displays the wavelength and power of the highest peak or an arbitrary peak using large easy to read numbers. This allows the values to be easily read even if the unit is placed at the top of the test stand.



### • Multi wavelength mode

The multi wavelength mode displays a list of wavelength and power of multiple peaks with the wavelength and power of the highest peak or an arbitrary peak on top of the list. There is also a mode to show the list only to maximize the number of channels shown on the screen.



The horizontal bar graph easily identifies the optical power variation and flatness of the signal.

### • Delta wavelength mode

The delta wavelength mode calculates and displays the difference between a reference peak and the other peaks in terms of wavelength and power. This mode helps determine the peak spacing.

### • Grid mode

Displays the deviation between a set grid wavelength and a measured wavelength which is within a set search area centering the set grid wavelength.

Ne.	GRID WL[Fm]	PEAK WL[rm]	DEVINMI	EW (caBm ) 🔺
90	1549.3150	1549.3146	-0.0004	-8.76
89	1550.1161	1550.1008	-0.0153	-7.89
88	1550.9180	1550.9428	0.0248	-8.67
87	1551.7208			
86	1552.5244	1552.5241	-0.0003	-9.30
85	1553.3288	1553.3272	-0.0016	-9.41
84	1554.1340	1554.1345	0.0004	-9.20
83	1554.9401	1554.9396	-0.0005	-7.60
82	1555.7471			

### Optical spectrum view

The AQ6150 series can display an optical spectrum waveform obtained from a Fast Fourier Transform (FFT) algorithm. It allows for determining test conditions and troubleshooting an error in the measurement while confirming the actual spectrum.

When a peak is selected on the list, the peak automatically shifts to the center of the optical spectrum view, making viewing easy and convenient.



### Various measurement units

The measurement units can be chosen from:

 Wavelength: Wavelength (nm), Frequency (THz), or Wave Number (cm<sup>-1</sup>) • Power: dBm, mW, or µW

# **User-friendly interfaces**

- Easy-to-view bright color LCD
- Proven design and operability

The AQ6150 series' screen design and intuitive operability is inherited from YOKOGAWA's best selling optical spectrum analyzer. This interface has been proven by a vast population of users on a global scale in areas such as R&D testing and troubleshooting in manufacturing.

- USB ports
- For USB compatible data storage devices, mouse and keyboard.
- File function enables users to save data and screenshots to the internal memory or USB storage to use when creating test reports. Screenshots can also be saved by simply pressing the Print Screen button (PRT SCN) located on the front panel.



# **Efficient measurement & analysis functions**

The AQ6150 series is equipped with automatic measurement and analysis functions. These functions save valuable time and resources from creating/validating remote control and analysis programs.

### • Drift analysis

The drift analysis measures the variation of wavelength and power for each peak over time by repeating the measurement. It obtains maximum value(MAX), minimum value(MIN), and variation (MAX-MIN). This function is useful for long-term stability testing and evaluating the temperature dependency of lasers.

### Average measurement

The Average measurement obtains an average wavelength and power for each peak by repeating the measurement. This function helps reduce uncertainty of measurement for a modulated signal or unstable signals.

### Fabry-Perot laser analysis

The evaluation parameters of a Fabry-Perot laser can be analyzed and displayed instantly from the measured optical spectrum. Results includes:


Center wavelength, total power, spectral-width (FWHM), mode spacing, etc.

### • Data Logging function


Up to 10000 points of measurement data per channel can be stored and displayed in tabular or graph form.


It facilitates the long term stability test and temperature cycle test.

- conditions, execute an analysis, and modify the optical spectrum view.
- shifted by a simple click and drag. The peak threshold line, threshold for peak detection, can also be moved in the same manner.

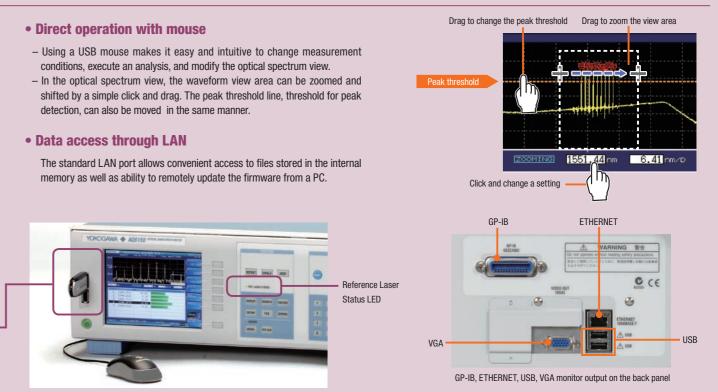

# AQ6150 series Optical Wavelength Meter

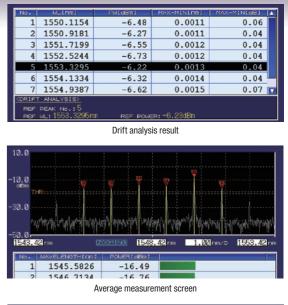



Fabry-Perot laser analysis

• Lasers / optical transceivers

requires high wavelength accuracy.

transceivers and transponders.

lasers

technoloav.

Testing of optical components used in WDM

transmission systems such as laser devices,

laser modules, and optical transceivers also

- Precise adjustment and inspection of tunable

- Modulated signal measurement of optical

- Measurement of all channels of 40G and


100G optical transceivers with WDM

# **Applications**

### • WDM transmission systems

In order to meet the rigorous demands of current and next generation communication networks, developers are constantly challenged to improve the efficiency and capacity of the transmission system. In response to these challenges, various techniques have been developed, such as minimizing channel spacing, maximizing the number of channels and transmission rate, using sophisticated modulation schemes, etc. In WDM transmission system testing, high wavelength accuracy is required for testing the system's internal circuit boards such as laser modules and optical transceivers as well as the final output signal of the system.

- Simultaneous measurement of multi channel and narrow spacing WDM system
- Precise adjustment and inspection of laser sources
- Measurement of modulated signals

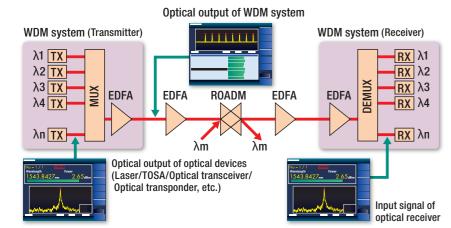

# **Principle**

### • Michelson interferometer

Generate interference by changing the optical path length difference between the fixed mirror and the movable mirror. Then detect the interference signal with the optical receiver.

### • Fast Fourier transform


Convert the interference signal into optical spectrum waveform.

### Fast data processing

Analyze the given optical spectrum waveform. Then output the wavelength and power data of the input signal.

### • Real-time wavelength correction


Correct the measurement error by simultaneously measuring the interference signal of the reference wavelength while measuring the input signal.

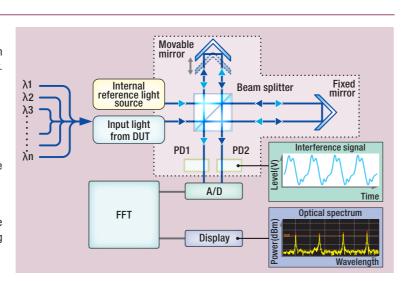

### • Calibration of test systems

Due to the high accuracy of the AQ6150 series, it can be used for precision wavelength calibration applications such as:

- Calibration of optical spectrum analyzers
  Calibration of DFB lasers for optical amplifier test system.
- Calibration of tunable lasers for passive component test systems.



The AQ6370 Series Optical Spectrum Analyzer commended for Side Mode Suppression tio (SMSR) of lasers and Optical Signal to Noise Ratio (OSNR) of WDM

# Major specifications

Items		A
Applicable optical fibe	er	SM (ITU-T G.652)
	Wavelength range	1270 to 1650 nm
Wavalanath	Wavelength accuracy *1	±0.7 ppm (±1 pm at 1550
Wavelength	Minimum resolvable separation *4	5 GHz (40 pm at 1550 nm
	Display resolution	0.0001 nm
	Power accuracy *2	±0.5 dB (1550 nm, -10 dł
Device	Linearity *2	±0.3 dB (1550 nm, -30 dł
Power	Polarization dependency *4	±0.5 dB (1550 nm)
	Display resolution	0.01 dB
Maximum number of	wavelengths	1024
Minimum input power		-40 dBm (1270 to 1600 n -30 dBm (1600 to 1650 n
Maximum input powe	r	+10 dBm (total of all lines
Safe maximum input	power	+18 dBm (total of all lines
Return loss *4		35 dB
Measurement time *3		0.3 s or less (single meas
	Measurement	Single, repeat, average, d
	Measurement condition setup	Average count, air/vacuur
	Display	Single wavelength, multin frequency (THz)/wave nur 1024 points), label, power
Functions	Data analysis	Peak search, FP-LD analy
	File	Saving/loading measured
	Remote control	Interface selection (GP-IB/
	Others	Internal reference light so initialization, firmware up
Display *5		5.7-inch color LCD (640×
Data storage		Internal: 256 MB or more,
Interfaces		GP-IB, ETHERNET, USB, VO
Remote control		GP-IB, ETHERNET
Optical connector		FC/PC or SC/PC (AQ9441
Warm-up time		60 minutes or more
Power requirements		100 to 240 V AC, 50/60 Hz
Environmental conditions		Performance guarantee te humidity: 20 to 85%RH (n
Dimensions and mas	\$	Approx. 426 (W)×132 (H)>
Safety standards		EN61010-1
	Laser	IEC 60825-1 Class 1
	Emission	EN61326-1 Class A, EN55
EMC	Immunity	EN61326-1 Table 2
RoHS		EN50581
Recommended calibration period		1 year
		+ ·

\*1 Line spectrum, CW, constant polarization during measurement, vacuum wavelength, input power confidence level (k=3)

\*2 Line spectrum, CW, excluding polarization effects

\*3 Number of detected wavelengths 128 or less

\*4 Typical

\*5 Lipided crystal display may include a few defective pixels (within 0.02% with respect to the total number of pixels including RGB). There may be a few pixels on the liquid crystal display that do not emit all the time or remains ON all the time. These are not malfunctions.



150	AQ6151		
n)	±0.2 ppm (±0.3 pm at 1550 nm)		
ual power lines input)			
or higher)			
• ,			
single line input)			
single line input)			
nent)			
data logging			
avelength, device type (CW/mod	ulated), measurement range		
• • • • • •	vith zooming), wavelength axis units (wavelength (nm)/ m/mW/µW), center wavelength, total power, marker (up to sages, system information		
drift analysis, WDM (OSNR) anal	ysis		
ults (CSV), saving/loading setup	parameters (binary), saving screen images (BMP)		
ernet), TCP/IP configuration, rem	note monitor		
e on/off, internal reference light ng	source status LED, optical power offset, parameter		
dots)			
ernal: USB			
utput			
versal adapter)			
oprox. 100 VA			
	emperature: 5 to 35°C, storage temperature: -10 to +50°C,		
,	nsation) ) mm (excluding protrusions), approx. 11 kg		
	mm (excluding protrusions), approx. 11 kg		
Class A Group 1			
CD-ROM (user's manuals): 1, Ge			
-30 dBm or more, line separatior	n 10 GHz or more in case of multi-line measurement,		



# **Ordering information**

### Models and Suffix codes

Model	Suffix	Descriptions	
AQ6150		AQ6150 Optical Wavelength Meter	
AQ6151		AQ6151 Optical Wavelength Meter	
Spec code	-10	Base model	
Power cord	-D	UL/CSA standard	
	-F	VDE standard	
	-R	AS standard	
	-Q	BS standard	
	-H	GB standard	
	-N	NBR standard	
Optical	/FC	AQ9441(FC) Universal Adapter	
connector (Factory option)	/SC	AQ9441(SC) Universal Adapter	

### Accessories

Name	Model	Descriptions
Name	mouer	Descriptions
AQ9441 Universal adapter	813917321-FCC	FC type
	813917321-SCC	SC type
Rack mount kit	751535-E3	19-inch

AQ6150 series

**Optical Wavelength Meter** 

# **Related products**

# **Optical Spectrum Analyzer** A06370D

High performance optical spectrum analyzer optimized for Telecom wavelengths



- Wavelength range: 600 to 1700 nm
- Resolution: 0.02 nm
- Sensitivity: -90 dBm
- Dynamic range: typ. 78 dB



# **Multi-Application Test System** A02200 Series

Flexible and space efficient

Comprehensive test solution for optical components and systems



Mainframe (3-slot/ 9-slot)

- Module lineup: Optical light source/ Optical power meter/ Optical attenuator/ Optical switch/ Optical transceiver test
- · Built-in test applications & macro programming function

\* Any company's names and product names mentioned in this document are trade names, trademarks or registered trademarks of their respective companies.

\* "Typical" or "Typ." in this document means "Typical value", which is for reference, not guaranteed specification.

Copyright © 2012, Yokogawa Meters & Instruments Corporation

YMI-ME-MI-SE01

[Ed: 03/b]

okogawa

### YOKOGAWA METERS & INSTRUMENTS CORPORATION

Global Sales Dept. /Phone: +81-422-52-6237 Facsimile: +81-422-52-6462 E-mail: cs\_meter@cs.jp.yokogawa.com

YOKOGAWA CORPORATION OF AMERICA YOKOGAWA EUROPE B.V. YOKOGAWA SHANGHAI TRADING CO., LTD. YOKOGAWA ELECTRIC KOREA CO., LTD. YOKOGAWA ENGINEERING ASIA PTE. LTD. YOKOGAWA INDIA LTD. YOKOGAWA ELECTRIC CIS LTD. YOKOGAWA AMERICA DO SUL LTDA. YOKOGAWA AUSTRALIA PTY. LTD. YOKOGAWA MIDDLE EAST & AFRICA B.S.C(c)

Phone: +1-770-253-7000 Phone: +31-88-4641000 Phone: +86-21-6239-6363 Phone: +82-2-2628-3810 Phone: +7-495-737-7868 Phone: +55-11-5681-2400 Phone: +61-2-8870-1100 Phone: +973-17-358100

Facsimile: +1-770-254-0928 Facsimile: +31-88-4641111 Facsimile: +86-21-6880-4987 Facsimile: +82-2-2628-3899 Phone: +65-6241-9933 Facsimile: +65-6241-2606 Phone: +91-80-4158-6000 Facsimile: +91-80-2852-8656 Facsimile: +7-495-737-7869 Facsimile: +55-11-5681-4434 Facsimile: +61-2-8870-1111 Facsimile: +973-17-336100

Subject to Change without notice.

Printed in Japan, 603(KP)