



Atomic Absorption Spectrophotometers





AA-7000 Series

Atomic Absorption Spectrophotometers


Reaching Even Greater Heights

Enhanced Flame Analysis World-Class High-Sensitivity Furnace Improved Dual Atomizer System Advanced Safety Technology



System Configuration can Evolve with Your Needs

The AA-7000 Series can be upgraded by adding units to allow the system to handle the analysis targets.

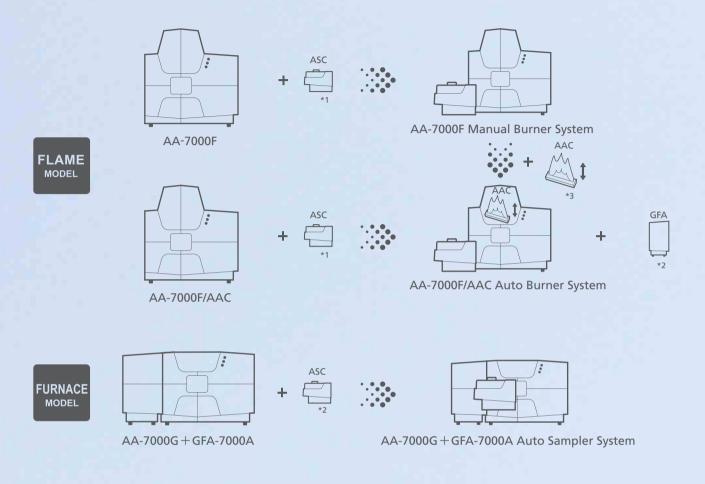


Analysis Sensitivities

Major Fields of Application

AA-7000 Series supports a wide range of analysis applications.

Environment





Metals, Semiconductors, Ceramics Metals, minerals, glass, ceramics, IC chips



Petroleum, Chemicals, Polymers Petroleum, oil, catalysts, chemical products, biodiesel

Medical, Biology, Pharmaceuticals Blood, animals, plants, drugs, food products

									Flam					Furn	200		
																1	
	Concentration limit of detection <							<0.01	0.01 ~0.09	0.1 ~0.9	1~ (ppm)		<0.01	0.01 ~0.09	0.1 ~0.9	1~ (ppb)	
Н																	He
Li	Be											В	С	N	0	F	Ne
Na	Mg											Al	Si	Р	S	Cl	Ar
K	Ca	Sc	Ti	V	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr
Rb	Sr	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	Ι	Xe
Cs	Ba	La	Hf	Ta	W	Re	Os	Ir	Pt	Au	Hg	Tl	Pb	Bi	Po	At	Rn
Fr	Ra	Ac															
				Ce	Pr	Nd	Pm	Sm	Eu	Gd	Tb	Dy	Ho	Er	Tm	Yb	Lu
				Th	Pa	U	Np	Pu	Am	Cm	Bk	Cf	Es	Fm	Md	No	Lr

* May differ according to coexisting substances in the sample.








AUTO /:

AA-7000F/AAC Dual Atomizer System



Autosampler

AUTO Dual Atomizer System Automatic adjustment of atomizer Automatic serach of burner height

Flame and Measurement Procedures

- *1 Requires ASC stand kit. *2 Requires ASK-7000.

*3 Automatic burner height search function can be used. AA-7000F/AAC equips with AAC as standard.

ASC

Flame Selection

														Air-C2H2	N2O-C2H2	HVG	MVU
Н								e									He
Li	Be											В	С	N	0	F	Ne
Na	Mg											Al	Si	Р	S	Cl	Ar
K	Ca	Sc	Ti	V	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr
Rb	\mathbf{Sr}	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	Ι	Xe
\mathbf{Cs}	Ba	La	Hf	Ta	W	Re	Os	Ir	Pt	Au	Hg	Tl	Pb	Bi	Po	At	Rn
Fr	Ra	Ac															
				Ce	Pr	Nd	Pm	Sm	Eu	Gd	Tb	Dy	Ho	Er	Tm	Yb	Lu
				Th	Pa	U	Np	Pu	Am	Cm	Bk	Cf	Es	Fm	Md	No	Lr




AA-7000F Flame Model





Enhanced Flame Analysis

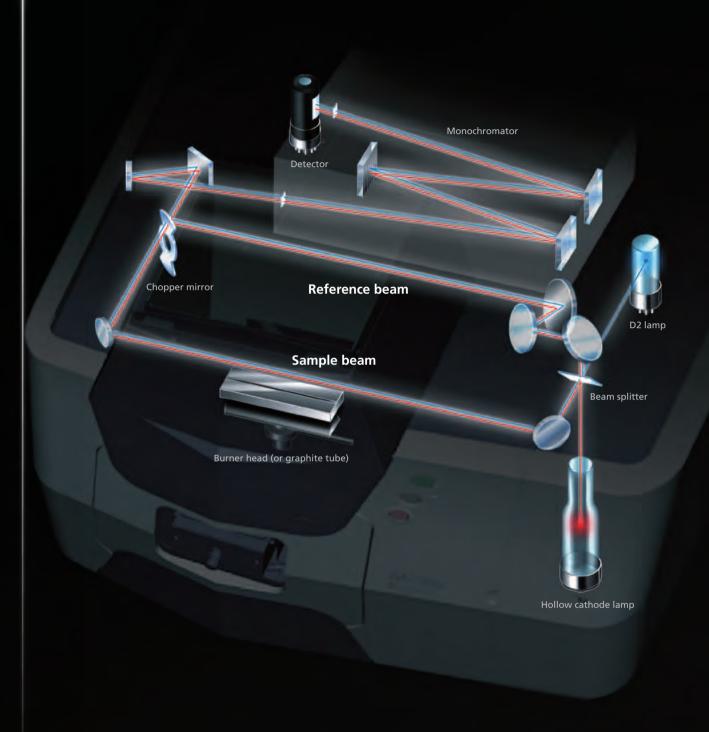

Double-Beam Optics and Stable Hardware Achieve Superior Stability


The AA-7000 Series incorporates newly developed 3D double-beam optics.

The optical system has been designed to produce its maximum performance for each measurement method through optimal adjustment of the light beam and light beam digital filter, and by using optical components that restrict light losses.

Advantages of the Double-Beam System


Long-term stability

The graph shows the results of measurements on 2 ppm copper (Cu) conducted over at least one hour. (The plot shows mean values for 11 repeated measurements.) Over the course of more than 600 measurements, the instrument achieved a relative standard deviation within 1%.



High sensitivity

The graph shows the direct measurement results for 0.1 ppm lead (Pb).



0.1 ppm to 0.4 ppm Calibration Curve for Lead (Pb)

0.100

ank Meat ST

0.100

0.00

Support for Developing Analytical Conditions

Automatic gas flow rate optimization

Automatic searching for optimal fuel gas flow rate (Japanese Patent 2099886). It is important to determine the optimal gas flow rate for the flame when using an organic solvent or after changing the burner height. The AA-7000F Series automatically optimizes the gas flow rate by measuring the changes in absorbance between a blank and a standard sample. The difference between the two is displayed on the screen. The gas flow rate achieving the highest sensitivity is detected and this value is automatically set as the gas flow rate value.

Automatic burner height optimization (AA-7000F/AAC)


The absorption sensitivity for flame analysis is also affected by the burner height. This results from variations in the flame temperature due to the burner height. The flame temperature is also affected by the matrix components. AA-7000F/AAC adjusts the burner height in 0.5 mm steps to automatically search for the optimal conditions.

AA-7000F enables above function by AAC-7000 (option).

Optional Autosampler Reduces Analysis Workload

Low carryover

Great care must be taken to avoid carryover during flame analysis. The new ASC-7000 autosampler rinses the nozzle at the rinsing port on the overflow mechanism after each sample measurement is complete. This ensures 10⁻⁴ max. carryover during the measurements of multiple samples. The graph shows the results of consecutive analyses of 10 ppm, 20 ppm, and 50 ppm sodium (Na) standard solutions in the EMISSION mode. No carryover could be detected when measuring the 10 ppm standard sample immediately after the measuring the 50 ppm Na standard sample.



Conventional method Overflow method

Data showing low carryover

Trace Sample Analysis Using Micro Sampling

Micro sampling

At least 1 mL (1000 μ L) volume of a liquid sample is required for the continuous intake of sample during normal flame analysis. With micro sampling, however, approximately 50 to 90 μ L of sample is injected in one shot into the flame and quantitation is based on the height and area of the peak signal obtained. This method offers the advantages below.


Advantages

- Permits analysis of small sample volumes
- Multi-element analysis of small sample volumes
- $\boldsymbol{\cdot}$ No blockage of burner slot with samples having a high salt concentration
- Synchronized with the autosampler for auto-dilution measurements
- * Synchronization with the autosampler requires the optional micro sampling kit.

Example of micro sampling analysis

Examples of the measured waveforms (overlaid) and calibration curve for micro sampling analysis are shown to the right.

A 2-ppm Cu standard solution was prepared by auto-dilution using the autosampler. The autosampler can also be used to conduct dilution measurements of the sample. (Injection volume: 90 μ L)





AA-7000 Series World-Class High-Sensitivity Furnace

Achieves World-Class Lower Limits of Detection

Advances in optics and a new graphite furnace design achieve improved lower limits of detection for furnace analysis (comparison with previous Shimadzu models).

This superb analysis performance is possible in all fields.

Enhanced Sensitivity	/ due	to	Graphite	Furnace
----------------------	-------	----	----------	---------

Previous	New
Pb 0.08ppb	0.05ppb
Mn 0.02ppb	0.01ppb

High-Performance Autosampler

- Mix and inject up to four sample types (diluted solution, standard solution, sample, matrix modifier, etc.). (Of course, unmixed samples can also be injected.)
- Select a fluororesin tube or pipette tip as the injection nozzle.
- Automatic dilution and re-analysis if the calibration curve concentration is exceeded.




Example of Automatic Dilution and Re-Analysis

Analysis of cadmium (Cd): The maximum concentration of the calibration curve has been set to 1ppb. At 1.8ppb, the sample of [003] has exceeded the maximum concentration. As a resultit has been automatically diluted by 4 times and re-measured.

1			A CONTRACTOR OF					No.	N. 5		_		and the second s	
-	Action	Sample ID	True Value (ppb)	Conc. (ppb)	Abs	Pos	VOL	Diluent R1	Reagent 1 R2	Total Volume	ASC DF	Actual Conc.	Actual Conc. Unit	Out of Control Remark
19	SPIKE1-2	001+@	0.2500	0.7661	0.3089	4	10	3	3	20	1. A	0.7661	ppb	
20	SPIKE1-A	001+@	0.2500	0.7558	0.3048	4	10	5	5	20	1	0.7558	ppb	
21		(K			1.00	1				- N	1			
22	1997-201	1		1	1	1			1	- 27	1		-	-
23		100		-		5	-	0	- 11	20			1000	2008 1 1 4000
24	UNK3-1	003		0.5231	0.2123	5	5	15	0	20	4.0000	2.0924	ppb	
25	UNK3-2	003		0.5047	0.2050	3	3	15	0	20	4,0000	2,0185	ppb	
26	UNK3-AV	003		0.5138	0.2086	5	5	15	0	20	4 000	2 0552	ppb	

High-Sensitivity Application Data (Analysis of Selenium (Se))

Independent control of the gas flow through the graphite tube during atomization achieves extremely high-sensitivity measurements. (Japanese Patent 2067563)



0.100	E 001.0	0100	0100	0100
0.090	0.090	0.090	0.090	0.000
0.000	0.000	0.000	0.000	0.000
0.070	0.070	0.070	0.870	11.070
0.060	0.060	0.000	0.060	0.000
0.050	0.050	0.050	0.050	0.050
0.040	0.040	0 040	0.040	0.040
0.000	0.000	0.000	0.000	0.000
0.020	0.020	0.020	0.020	0.020
000	0.010	0 010	0.010	0.000
0.000	10.000	0000	0.000	0.000
ama 1	ann Herter	ama 25	amatin	ama

Measurement Example Showing High Sensitivity


Analysis of 0 to 5 ppb selenium (Se): Sensitivity is adequate for 1 ppb measurements. (20 μ L injected volume, Pd modifier, pyro-coated graphite tube)

Digital temperature control and electronic gas flow control enhance stability

Combination of a high-sensitivity optical sensor and unique digital temperature control technology achieves highly accurate temperature control in all temperature regions from drying to atomization. An electronic flow controller can precisely control the inner gas flow rate in 0.01 L/min units. These control techniques significantly enhance both the sensitivity and the data stability.

Measurement Example Showing High Stability

Analysis of 0.5 ppb lead (Pb): Approx. 5% relative standard deviation after 5 repeated measurements is adequate for quantitative analysis.





High-density graphite tube (P/N 206-50587) Can be used for all elements. Especially effective for low-boiling point elements (Cd, Pb, Na, K, Zn, Mg, etc.).



Pyro-coated graphite tube (P/N 206-50588) Effective for elements that readily form carbides (Ni, Fe, Cu, Ca, Ti, Si, V, Mo, etc.).




Platform tube (P/N 206-50887-02)

Restricts chemical interference due to coexisting substances. Effective for the analysis of environmental samples and biosamples, such as sea water and industrial waste.

* Depending on the state of the sample, some other combinations may be appropriate.



Improved Dual Atomizer System

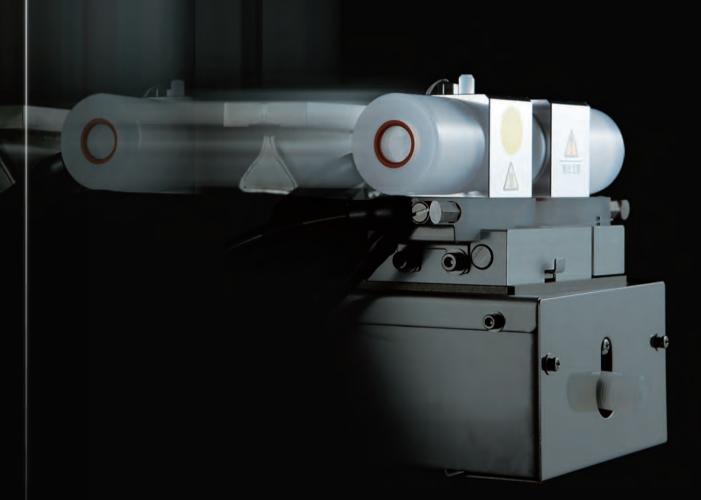

Single Unit Handles High Concentration to Trace Analysis Samples

AA-7000F/AAC creates an integral burner and furnace that remains permanently installed in the combustion chamber. It supports both flame analysis of high concentration samples and furnace analysis of trace samples, without changing the atomizer unit. The integral construction with the atomizer saves space. AA-7000F enables above function by AAC-7000 (option).

* The AAC-7000 cannot be attached to an AA-7000G instrument.

New Atomizer Design Permits Easy Switching Between Flame and Furnace Measurements

- The new drive mechanism halves the switching time between flame and furnace measurements (comparison with previous Shimadzu models).
- The atomizer unit is switched automatically by software operation. No troublesome replacement of the atomizer unit is required. No need to disconnect pipes or wires.
- In case of the flame measurement of high-concentration sample, offsetting the burner head from the light axis, instead of angle adjustment, allows to adjust the sensitivity.
- A single autosampler can be used for both flame and furnace measurements. Simply slide it left or right. No need to purchase two autosamplers.



Smallest footprint for a full system

The system with a dual atomizer fits into a 960 mm width (including power supply for the graphite furnace atomizer), achieving the world's smallest installation footprint* for a full system.

* Shimadzu in-house investigation. Current as of November 2008.



Flame measurement: Burner head intersects the light axis (red line).

Furnace measurement: Furnace intersects the light axis (red line).



Flame measurement



Furnace measurement

Easily attach an autosampler

Direct connection of the autosampler to the AA instrument minimizes the installation footprint and simplifies maintenance.




Lamp house

Just slide the cover to the side for easy replacement of the hollow cathode lamps through the large opening.







* Dimensions do not include ASC-7000. Height (H) does not include protrusions.




Advanced Safety Technology



Comprehensive Safety Functions in Every System

Safety is an extremely important consideration for flame atomic absorption spectrophotometers using acetylene gas. The AA-7000 Series instruments are the first* ones in the world fitted with a vibration sensor as standard. They also incorporate a comprehensive range of safety mechanisms, including gas leak detectors.

* Shimadzu in-house investigation. Current as of November 2008.

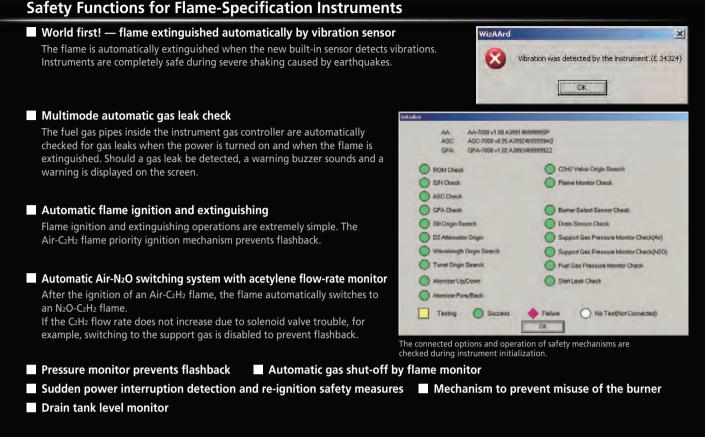

Safety Functions for Furnace-Specification Instruments

- Cooling water flow rate monitor Argon gas pressure monitor Furnace cooling check
- Overcurrent protection unit (double-checked by circuit protector and optical sensor)

Safety-Conscious Design

Flame-retardant materials

UL 94V-0-rated flame-retardant materials are used for the instrument external covers and atomizer unit. This superior design pays due consideration to safety.

Safe ignition switches

The switches perfectly fit finger contours and are positioned near the window.

To prevent inadvertent operation, both switches must be pressed simultaneously to start ignition.

Durable pipes and reliable couplings

All pipes are selected for durability and used with highly reliable couplings.

Clear window

The large window permits observation of the flame, and the burner can be easily accessed through the large opening. The window closes when released to eliminate the chance of it being left open.







Dual-Background Correction Functions

The optimal background correction methods are installed as standard: high-speed self-reversal method (SR method) and deuterium lamp method (D₂ method).

These functions can correct for spectral interference in flame measurement. Selecting the optimal background correction method for each sample ensures accurate and reliable analysis results.

Samples suitable for the SR method


Samples with a complex matrix (Containing a large quantity of a specific element as the main component) Samples suitable for the D2 method

Purified water, tap water, environmental water, etc. Samples with a relatively simple matrix

SR (high-speed self-reversal) method — accurate background correction over a wide range

Features


- 1. High-speed self-reversal (SR) correction is generally more accurate than deuterium lamp (D₂) correction. As both atomic absorption and background absorption can be measured using a single lamp, the correction errors due to light-axis misalignment are extremely small. This is ideal for the quantitation of trace components in a matrix exhibiting complex background absorption, such as bio-samples and metals.
- 2. Permits background correction over the entire wavelength range from 185 nm to 900 nm.
- 3. This method can correct for spectral interference due to neighboring lines that can occur when a resonance line for another element exists near the analytical line for the target element. (See table on next page.)
- 4. As no polarizer is used, measurements are possible with low light losses and a high S/N ratio.
- 5. The rapid lamp lighting permits accurate measurement unaffected by emission noise in the atomizer.
- * Hollow cathode lamp L-2433 is required to use the SR method. Hollow cathode lamp L-2433 can also be used for the D2 method.

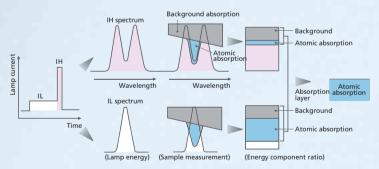


Principle

A small current IL (approx. 10 mA) and a large current IH (approx. 500 mA) are alternately passed through the hollow cathode lamp. The lamp emission spectrum when the large current flows has a depression in the center (self-reverse), due to self-absorption of the large number of sputtered atoms in the atom cloud, as shown in the diagram to the left. No significant atomic absorption is apparent and background absorption mainly occurs. Conversely, the lamp emission spectrum when the small current flows comprises a single narrow peak resulting from both atomic absorption and background absorption. By determining the difference between the two types of absorption, it is possible to accurately correct for the background absorption and measure the true atomic absorption.

Examples suitable for SR method (where differences result between SR and D² **methods)** Example: Measurement of trace levels of zinc in iron (analysis of Zn in Fe solution)

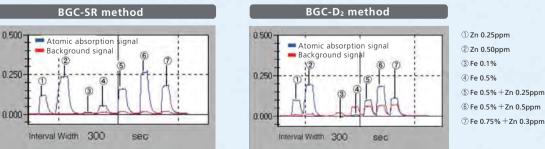

The identical 0.5 ppm Zn solution is accurately corrected to the same absorbance at (2) and (6).



Examples of	elements	and	wavelengths causing spectral
interference	problems	due	to neighboring lines


Measured Element	Analytical Line (nm)	Coexisting Element	Absorption Line (nm)
AI	309.28	Mg	309.30
As	193.76	Fe	193.73
Ca	422.67	Fe	422.64
Cd	228.80	Ni	228.84
Cu	324.75	Fe	324.73
Ga	294.36	Ni	294.39
Mg	285.21	Fe	285.18
Ni	232.00	Fe	232.04
Pb	217.00	Fe	216.95
Sb	217.58	Fe	217.55
Se	196.03	Fe	196.05
Si	251.61	Fe	251.69
Zn	213.856	Fe	213.8589

The SR method is suitable for samples containing elements that cause problems with spectral interference, as shown in the table to the left.

D₂ (deuterium lamp) method — highly sensitive background correction

Features

- 1. Detection sensitivity is superior to the SR method. Therefore, this method is suitable for the analysis of samples with a simple matrix requiring high sensitivity, such as the measurement of trace levels of impurities in ultrapure water or environmental analyses.
- 2. As the lighting frequency is higher than with the SR method, it can eliminate noise due to emission components of the flame or graphite tube to permit accurate atomic absorption measurements.
- 3. The original hollow cathode lamp can be used.




Principle

The deuterium lamp method involves lighting the hollow cathode lamp and the deuterium lamp alternately at high speed. After separation by the monochromator, the light from the deuterium lamp has a bandwidth from 0.1 to 5 nm. Therefore, an atomic absorption with a line width of only about 1/1000 nm is almost unobservable compared to the background absorption due to wide-bandwidth molecular absorption. However, as the light from the hollow cathode lamp has approximately the same bandwidth as the atomic absorption band, the total of the atomic absorption and the background absorption can be observed. With the deuterium lamp (D₂) method, light from both sources passes through the atomizer. The difference in absorbance is determined to conduct background correction.

Examples suitable for D₂ method (where no difference results between SR and D₂ methods)

Example: Measurement of trace levels of lead in 2% NaCl solution by molecular absorption (analysis of Pb in 2% NaCl solution)

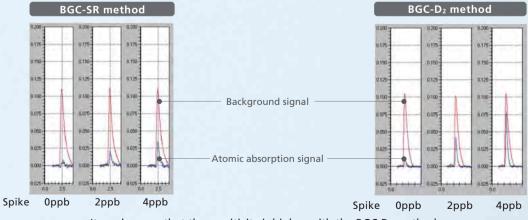


It can be seen that the sensitivity is higher with the BGC-D₂ method.

AA-7000 Series Clear, Easy-to-Use Software


Features of the WizAArd Software

The WizAArd software used with the AA-7000 runs under Windows 7/Vista/XP.

Wizard Functions Make Setting the Conditions So Simple That Even a Novice Can Do It.

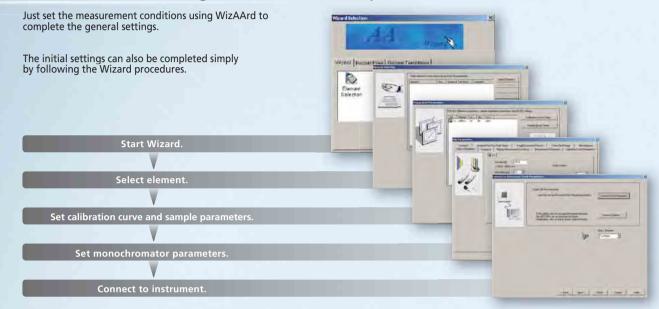

Measurement Screen Layout Shows Measurement Status at a Glance

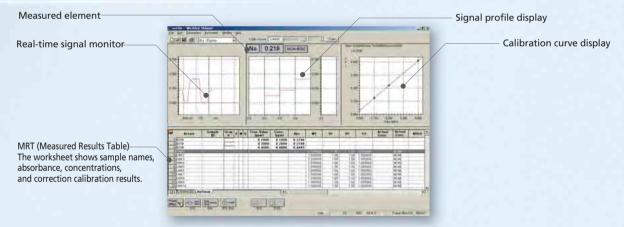

Lamp History Function Assists with Lamp Management


The accumulated operation time for each lamp displayed on the lamp registration screen assists with lamp service life management. Multiple lamps for the same element are differentiated using lamp IDs.

	Lump III	Elument	Lamp	Life Time	time Time	tise.	Judge	Comment	Lock -	-94
1.	U2		62	500	0.0	firs:	OK.		T-	
2.1	Aget	Ag.	t-trame.	5000	0.0	mA/YES	OK		F	Cence
5	AL4	N	Nurmial	5000	0.0	mAmeri	OK.		F	
6	As.t	.A3	Nume	3000	0.0	mA'fen	OK		Г	Claim
5	Aut	JAN .	Alternation	5000	0.0	mA*rrs	OK		17 1	
0	B-1		Nervel	5000	00	114.972	OK		E	Datain
1	Be-1	Bu	Normal	5000	0.0	mA.Tvs	CH		C	Berninin
8	Be-1	Đr	Name	5000	0.0	mAtes:	OK		C	Dist
9	15.1		SAUTTINE	5000	00	MATES.	CR6		E .	Ehint
10	CAT	64	Northill	\$500	0.0	mA.*ixs	CH		E	
10. 11.	Cd/t	Cd	Nontel	5000	0.0	#A?YA	CNI		E	
12	100-1	60	Normac	5000	0.0	10A7978	CH4		F	
13	01-1	- Gr	Skormel	5000	0.0	mATYS	CW		10	
14	Ctt-1	C#	Normal	5000	0.0	mA Yes	OK		T I	
15	Cu.i	ču	Normal	5000	0.0	mA free	OK		1	

Software Provides Comprehensive Information Displays and Flexible Settings


Identical software operation for flame and furnace measurements

- Even if the calibration curve is created after sample measurements, concentration calculations can be conducted on past data. This allows trial measurements to be directly used as actual measurements.
- Extrapolation of calibration curve range. If the sample concentration exceeds the calibration curve range, additional measurements can be performed on standard solutions to re-calculate the concentration.
- Ose existing calibration curves for measurements. Useful for sample concentration order checks and for checking the instrument sensitivity.
- ④ One-touch re-measurement operation. No need to repeat the measurement from the beginning.
- Create and save multiple calibration curves on a single worksheet. Select the appropriate calibration curve for the sample concentration and composition.

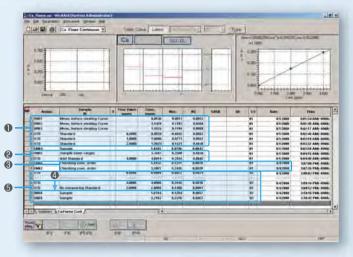

Combining a high-performance autosampler simplifies advanced settings

- Real-time drying and ashing progress display for furnace measurement
- A higher temperature cleaning operation than the cleaning stage can be added for each measurement. This reduces the graphite tube memory effect. Tube deterioration is reduced by minimizing the cleaning operations.
- SAdd optional autosampler rinsing operations to ensure adequate rinsing of the autosampler after completing the measurement of high-concentration samples.
- ④ Set up sample dilution and spike-and-recovery tests on the same screen.
- **⑤** Overlay function allows size and shape comparison of peak profiles.
- **6** Large-volume injection permits high-sensitivity measurements.
- Precision control of drying and ashing temperatures reduces analysis time.

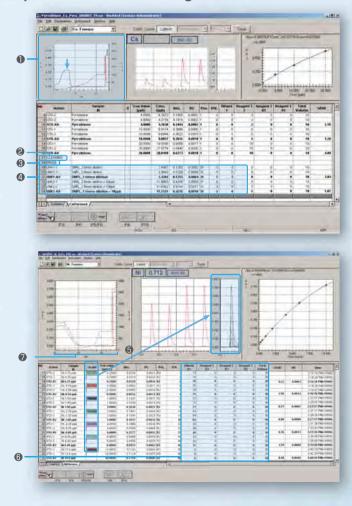

Supports System Management and Accuracy

FDA 21 CFR Part 11 Compliance

AA-7000 Series

- A combination of enhanced WizAArd software with Shimadzu's network-compatible CLASS-Agent data management software supports FDA 21 CFR Part 11 Compliance.
- WizAArd used alone provides comprehensive system policy setting, user management, log browser, audit trail, and electronic signature system management functions.
- Hardware validation software installed as standard.

Comprehensive Data Management Functions

stem Policy e system policy settings allow advanced ssword and lockout settings. The levels n be set in stages from "unrestricted" "Part 11 compatible".	CLASS-Agent (Option) Connection to CLASS-Agent permits efficient, long-term database management of large amounts of analysis data.
ride= Rider Setting = Almaubrakan	
Mennum Password Leasth Maximum Password Aas D Password Aas D	
Lockool Develors [15] inco Lockool Settler: Bor User) Lockool Settler: Bor User) Lockool Settler: Bor User to D	
	peration alidation System Folicy Agent Connection Setting
0	peration System Folicy Agent Connection Setting
Iser Administration XI	peration alidation System Folicy Agent Connection Setting
Seer Administration Seer Administration Secret Administration Secret Administration Secret Administration Secret Administration Administration Control and Adjust MWR Administration Revelopment	peration alidation System Folicy Agent Connection Setting User Administration Log Browser User Administration Log Browser Connection
Seer Administration Seer Administration Secret Administration Secret Administration Secret Administration Secret Administration Administration Control and Adjust MWR Administration Revelopment	peration alidation System Folicy Agent Connection Setting User Administration Log Browser

User management restricts the users of the system. It registers each user to determine how each one uses the

Log Browser The log browser easily displays a variety of logs to check the system modification history and other log information.

software.

Management

Accuracy Management (QA/QC) Functions Permit User Level Management, Audit Trail, and Electronic Signatures


QA/QC compatibility The QA/QC functions permit accuracy management.

R BY	70 .	- 110	8	1	Mpt & Co	ninar 🗶
P LV	10 .			1	Marisco	ntear *
P.E.B.	- 0	GREA		F	Mark & Ge	ntinue 🔹
P cov	00	. pin		F	Mart & Gu	ilene z
R COB	50	1:101		r .	Mark & Co	ninur 🦉
OGR DON	Trepency :	er Eto	-	mili	w 120	mulate
Augustine Par						
Mathed	Tran Value	Part	VE		Disest	Hanganal 3
	A LONG TO DO TO	A Provenile				112
100/100 m	£ 0000	- BE			2	



Hardware validation software installed as standard

The hardware validation software makes it simple to evaluate the instrument performance. When combined with the autosampler, it automatically determines the wavelength accuracy, noise level, baseline drift, absorbance and repeatability, and prints out the results of comparison with the pass criteria.

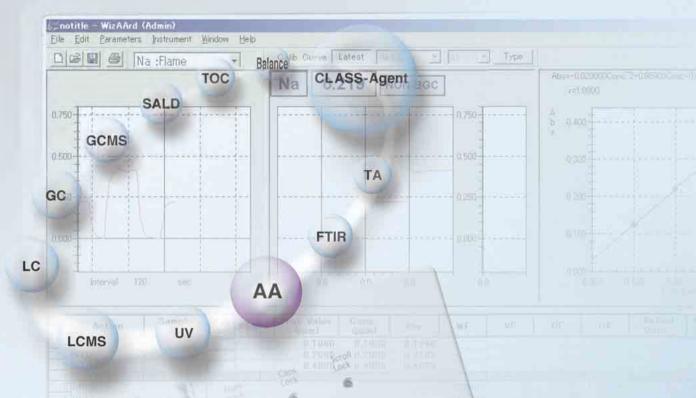

* Data from all Shimadzu analytical instruments can be centrally managed by CLASS-Agent.



AA-7000 Series Standard Parts / PC / Software

Common to All AA-7000 Series Models

Part Name	Quantity	P/N
Cable set	1	071-60821-08(120V),071-60825-51(230V)
Cards (set of 10)	1	206-52046-91
Instruction manual	1	206-97176
Safety inspection sheet (safety instruction)	1	206-97225
Declaration of conformity, explanatory notes (ISO-9001)	1	228-30164
Warranty label	1	037-70238-01
Registration form	1	221-40500
Serial number label	3	206-57770

* The PC, monitor, printer, hollow cathode lamps, high-temperature burner head, pressure regulator and compressor are not included in the standard configuration.

AA-7000F, AA-7000F/AAC Standard Parts List

Part Name	Quantity	P/N
Hose ASSY (for air supply)	1	206-50389-91
Hose ASSY (for C ₂ H ₂ gas supply)	1	206-50389-92
Hose clamp (16 mm)	2	037-61019
Cleaning wire	1	201-79229-01
Sampling tube (PTFE)	2	204-05899-01
Sampling tube (for organic solvent samples)	1	206-50772-91
Polyethylene tubing, No. 3	1 (0.3m)	200-31328-01
Polyethylene tubing, 8 × 1 (drain tubing)	1 (2.4m)	016-43201-02
Drain ASSY	1 1	206-77413-41
Grease (in cup)	1	206-50442-91
Funnel	1	206-77243-92
Declaration of conformity, English version (ISO-9001)	1 _ 1	206-84934-66/-68
Inspection report	1	206-77551-02/-22

AA-7000G Standard Parts List

Part Name	Quantity	P/N
Declaration of conformity, English version (ISO-9001)	1	206-84934-67
Furnace mounting plate	1	206-77704
Inspection report	1	206-77551-12

* GFA-7000A is not included in the standard configuration.

Personal Computer / Monitor

Microsoft Windows 7 Professional (32 bit) Vista Business or XP Professional
Intel® Celeron 420 (1.60 GHz) or higher
1 GB or higher (Vista) or 512 MB or higher (XP)
XGA (1024 × 768 dots) or higher
One CD-ROM drive (for installing software) Requires 60 MB min. hard disk space for installation
One serial port (for AA control)

* Windows is a registered trademark of Microsoft Corp., U.S.A.

Optional Accessories / Related Products

For Flame Analysis

Part Name	P/N	Remarks	
High-temperature burner head	206-77530-91	Made of pure titanium. Air-cooled. 5 cm slot for N2O-C2H2 flame	
T		•Extremely corrosion-resistant •Can also be used for Air-C₂H₂ flame.	
Flow meter kit	206-77617-91	Float-type flow meter for support gas	
Sample platform	206-77655-91	Dimensions: 250 W × 130 D × 170 H mm Vial mounting platform: 220 W × 95 D mm Vial positions: 5-step switching	
Air compressor	208-91753-91	100 VAC, 50/60 Hz, with mist separator	
Low-noise air compressor	208-91750-36	100 VAC, 50/60 Hz, with mist separator	
Mist separator kit	206-52458-91	Required if using an air compressor other than above.	
YR-71 compressed gas regulator	040-72020-01	For C ₂ H ₂	
MAF-85S compressed gas regulator	040-72019-11	For dinitrogen oxide gas	
Micro sampling kit	206-77540-91	Required to use the flame micro sampling method. ASC-7000 and ASK-7000 (or ASC stand kit) are also required.	
O-ring set	206-77620-92	O-ring set for organic solvents	

For Furnace Analysis

Part Name	P/N	Remarks	
GFA-7000A graphite furnace atomizer 206-77777-XX		 Specifications Heating control system: Drying: Digital current control (with automatic temperature calibration function) Ashing, atomization: Digital temperature control via optical sensor Heating temperature range: Ambient to 3000 °C Inner gas type: Dual automatic switching type Inner gas flow rate: 0 to 1.50 L/min, 0.01 L/min increments Ar gas: 3.5 L/min max. Cooling water: Cooling water circulation unit or tap for process water Water temperature: 10 to 30 °C, flow rate: 0.6 to 1.5 L/min * Separately order the parts below. 	
Graphite Furnace Camera GFA-TV	206-52950-91	Provides viewing inside the graphite tube. Including Video View Software (CD-ROM)	
High-density graphite tube	206-50587		
Pyro-coated graphite tube	206-50588	Select one of the three types of graphite tubes according to the aim of the analysis.	
Platform tube	206-50887-02		
MAF-106S compressed gas regulator	040-72019-21	For Argon gas	
CA-1114A-1 cooling water circulation unit	044-01809-07	For cooling GFA, 100 VAC, 1100VA, 50/60 Hz	
Parts for cooling water co	onnections		
Cooler connection kit	206-84373-91	For connecting GFA and CA-1112	
Cooling water tube ASSY	206-51028-91	Connecting tubes when using tap water to cool GFA	

Autosampler

Part Name	P/N	Remarks	
ASC-7000 autosampler	206-77600-XX	Specifications	
For flame analysis	For furnace analysis	System: Flame / furnace Function: Zero-point detection, auto rinse, auto diagnosis, random access Maximum reagent / sample positions: Reagents: 8 positions, samples: 60 posi * Separately order the parts below.	
ASC stand kit	206-77650-91	Required to mount ASC-7000 to conduct flame analysis only.	
ASK-7000 extension unit for furnace analysis	206-77550-41	Permits both flame and furnace analysis.	
Nozzle ASSY, HVG	206-67563	Required to use ASC-7000 and HVG-1.	



Optional Accessories / Related Products

Dual Atomizer System

Part Name	P/N	Remarks
AAC-7000 auto atomizer changer	206-77701-41	Required to add GFA-7000A to AA-7000F to conduct furnace analysis. Permits automatic burner position setting for flame analysis with AA-7000F.

Hollow Cathode Lamps

Part Name	P/N	Remarks
L-233 series	200-38422-XX	
L-2433 series	200-38456-XX	For SR method

Other Accessories

Part Name	P/N	Remarks
Analog output cable	206-77707-91	Used for analog output to a pen recorder, etc. One cable required per channel (atomic absorption/energy signal, background signal).

For High-Sensitivity As, Se, Sb Analysis

Part Name	P/N	Remarks	
HVG-1 hydride vapor generator 206-17143-XX		 Environmental standards prescribe the hydride generation method as one method of As, Se, and Sb analysis. 1. Used with the AA-7000 Series, HVG-1 permits the rapid and accurate quantitation of elements such as As, Se, Sb, Sn, Te, Bi and Hg at several-pp levels. 2. Used with an ASC-7000 autosampler, it permits the automated serial analysis of up to 60 samples. * Nozzle ASSY, HVG (PN: 206-67563) is required to use HVG-1 with an ASC-7000 Series instrument. Order separately. 	
		 Specifications Measurement method: continuous flow Sample consumption: 0 to 7 mL/min, variable Reagent consumption: 0 to 2.5 mL/min, variable Atomizer: Heated absorption cell (heated by Air-C:H₂ flame in standard system) Carrier gas: Ar pressure: 0.32 MPa, consumption: 70 mL/min Power requirements: 100, 115, 220, 240 VAC, 30 VA, 50/60 Hz Dimensions: 340 W × 220 D × 200 H mm Standard Major Items Hydride vapor generator, absorption cell (P/N: 206-77607) Reagent bottles (P/N: 204-09363-01), gas hose, drain tube, etc. 	

For Higher Sensitivity with the Hydride Generation Method

Part Name	P/N		Remarks
Part Name P/N SARF-16C atomic muffle furnace (Electronic Cell Heater) 208-97249		hydride vapor 2. The tempera temperature. 3. Good tempe damage due to	ed furnace permits higher sensitivity measurements using the generator than the flame heating method. ature controller provides optimal control of the quartz cell erature reproducibility. Extends cell life by preventing
Cel	I heater Controller	Specification Furnace	ns Dimensions: 170 W × 110 D × 110 H mm I.D.: ø25 × 170 mm Heater: PYROMAX DS
HVG-1 hydride vapor generator Atomic absorption spectrophotometer		Controller	Operational temperature range: Ambient to 1100 °C Temperature regulation range: ±2.5 °C Load capacity: 1000 W max. Power requirements: 100 VAC, 400 VA, 50/60 Hz
	200 52425 04		transformer in regions that do not have a 100 V power supply.
Mounting adaptor	206-52135-91	For AA-7000F	
	206-83755-91	For AA-7000G	

For High-Sensitivity Hg Analysis

ICP Emission Spectrometers



Remarks

Offers both high throughput and easy analysis. Does not require processing of large data volumes, such as spectral line selection, which was problematic with the conventional Multi-ICP. Various assistant functions allow anyone to rapidly perform accurate analysis.

Light source: Axial observation, compatible with mini torch Monochromator / detector: Echelle CCD Wavelength range: 167 to 800 nm (using vacuum monochromator)

AA-7000 series Specifications

Main Unit

Basics

	Wavelength range	185.0 to 900.0 nm
Optics	Monochromator	Aberration-corrected Czerny-Turner mounting, Number of grating grooves: 1800 lines / mm, Focal length: 300 mm
	Bandwidth	0.2, 0.7, 1.3, 2.0L nm (4-step automatic switching)
	Detector	Photomultiplier tube
	Optics	Optical double-beam
	Background correction method	 BGC-SR (high-speed self-reversal method) (185.0 to 900.0 nm) BGC-D2 (D₂ lamp method) (185.0 to 430.0 nm)
	Number of HC lamps	6-lamp turret, 2 lamps simultaneously lit (1 for measurement, 1 warming up for next measurement)
	Lamp mode	EMISSION, NON-BGC, BGC-D ₂ , BGC-SR
	Software requirements	Microsoft Windows 7 Professional / Vista Business / XP Professional
	Parameter setting	Wizard method
	Measurement mode	Flame continuous method, flame micro sampling method, furnace method, flame emission method
	Concentration computation mode	Calibration curve method (select primary, secondary, tertiary) Standard addition method, simple standard addition method (primary expression)
	Repeat analysis	Up to 20 repetitions. Mean value, standard deviation (SD) and coefficient of variation (RSD) display Automatic exclusion of deviant values by setting SD and %RSD
	Baseline correction	Automatic correction of baseline drift by offset correction in peak height / peak area modes.
	Signal processing segment setting	Signal processing segments can be changed in peak height / peak area modes.
	Sensitivity correction	Automatic calibration curve correction function using sensitivity monitoring
Data processing	Analog output	2 channels (atomic absorption/energy signal, background signal) Output range: 5.0, 2.5, 1.25, 0.625 Abs./V (each settable in 4 stages) Fixed at 1 V F.S. in EMISSION mode.
	Tabular data processing	Final concentration calculations based on sampled volume, dilution rate, fixed volume, and factor inputs
	Recall of parameters	Template functions available
	Procedure/result display	MRT (Measurement Results Table) worksheet
	Report generation	Summary report
	QA/QC	Select whether to continue or discontinue measurements based on results of evaluation on coefficient of correlation, %RSD, ICV·ICB, CCV·CCB, PB, LCS, SPK, PDS, and DUP.
	Re-analysis	 Select whether on not to conduct re-analysis. Automatic dilution and re-analysis of unknown samples via autosampler (flame micro sampling method, furnace method)
	Digital recording	Management by login ID and password • Control user access authority by user level • Log record • Audit trail • Electronic signatures
Power requirements		Choose from 100, 120, 220, or 230 VAC, 50/60 Hz (Power is required separately for the personal computer.)
Dimensions and weight		•AA-7000F/AAC: 700 W × 588 D × 714 H mm, 76 kg •AA-7000F: 700 W × 588 D × 714 H mm, 73 kg •AA-7000G: 700 W × 580 D × 538 H mm, 66 kg (Protruding parts and optional equipment are not included.)
Ambient temperature / humidity		10 to 35 °C, 20 to 80% (less than 70% when temperature is higher than 30 °C)

Flame

	Turne	Air sealed are mix tune	
	Туре	Air-cooled pre-mix type	
	Burner head	Titanium 10 cm slot (5 cm titanium slot for N2O-C2H2 flame available as an option)	
	Nebulizer	Pt-Ir capillary PTFE orifice eceramic impact bead (capable of handling hydrofluoric acid)	
	Chamber	Engineering plastics	
Burner unit	Positioning	•AA-7000F	
		Lateral/vertical manual adjustment	
		•AA-7000F/AAC	
		•Automatic flame/furnace switching by motor ·Automatic search of optimum burner height	
	Angle adjustment	0 to 90° (Angle adjustment is not possible if the optional GFA-7000A is installed on the AA-7000F/AAC.)	
	Туре	Air-C2H2 flame, N2O-C2H2 flame (Hydrogen flame is not applicable)	
Gas control	Flow rate control	• Automatic fuel gas flow rate setting (0.1 L/min step) • Automatic search of optimum gas flow rate	
	Safety measures	Automatic gas leak check •Automatic Air-N2O switching as C2H2 flow rate increases •Flame monitor •Prevention of wrong burner head use Gas pressure monitor •Drain tank level monitor •Automatic flame extinction upon power outage or sudden power interruption Automatic flame extinction via flame vibration sensor •Internal fan stop sensor	

Furnace (GFA-7000A)

Heating temperature range	Ambient to 3,000 °C	
Heating control system	Drying: Digital current control with automatic temperature calibration function Ashing, Atomization: Digital temperature control via optical sensor	
Optimum 20 stages • Heating mode: RAMP/STEP • Inner gas type: Dual automatic switching type •High-sensitivity mode setting •Enrichment in furnace: Maximum 20 times •Optimum temperature program search support function • Inner gas flow rate: 0 to 1.50 L/min		
Safety measures	Cooling water flow rate monitor · Gas pressure monitor · Overcurrent protection unit (double check by circuit protector and optical se Furnace block cooling check	
Positioning	•AA-7000G • Lateral/vertical manual adjustment •AA-7000F/AAC • Automatic flame/furnace switching by motor	
Power requirements	200, 220, 230, or 240 VAC ±5%, 7400 VA, 50/60 Hz	
Dimensions and weight 260 W × 560 D × 510 H mm, 47 kg		

Autosampler

Common Specifications

Control	RS-232C communication control from AA unit	
Maximum reagent / sample positions	Reagents: 8 positions Samples: 60 positions (random access available with reagents or samples)	
Rinse water bottle	21	
Power requirements	Choose from 100, 120, 220, or 230 VAC, 50 VA, 50/60 Hz	

Flame Continuous Method

Functions Zero-point detection, auto diagnosis, auto rinse, random access	
Sample volume Sample vials: 15 mL, reagent vials: 53 mL	
Nozzle rinse Solvent rinse aspiration method	
Dimensions and weight	Sampler: 340 W × 280 D × 270 H mm, 8 kg Controller (including stand): 260 W × 200 D × 320 H mm, 7 kg

Furnace Method / Flame Micro Sampling Method

Functions	Zero-point detection, auto diagnosis, auto rinse, auto mixing, random access	
Sample volume	Sample vials: 2 mL, reagent vials: 20 mL	
Nozzle rinse Solvent rinse discharge method		
Sampling functions Dilution function, reagent addition function		
Syringe 250 μL		
Injection volume 2 to 90 µL		
Repeatability 1%RSD (20 μL)		
Carryover	Rinse port: Less than 0.0001 Mixing port: Less than 0.00001	
Mixing port rinse	Solvent rinse discharge method, solvent discharge and rinse with next sample	
Mixing function Performed in mixing port. Maximum mixture volume: 0.6 mL		
Maximum number of mixing reagents added	Up to 4 solutions Number of solutions possible for mixing ·Calibration curve method: 5 solutions max. (sample + 4 types of reagents) ·Standard addition method: 6 solutions max. (sample + standard solution + 4 types of reagents)	
Auto dilution / re-analysis For measurement result on unknown samples: · If extrapolation of calibration curve is possible: automatic calculation of dilution rate and dilution to bring concentration within contract of the extrapolation of calibration curve is not possible: dilution rate fixed at 10x		
Dimensions and weight Sampler (including sliding parts): 340 W × 280 D × 400 H mm, 11 kg Controller: 235 W × 110 D × 240 H mm (built into GFA-7000A), 6 kg		

Required Software Operation Environment

Shimadzu recommends the PC and monitor in the PC Set for AA-7000 Series with WizAArd Software Pre-Installed. Purchase a printer separately. The personal computer and monitor specifications are as follows.

Operating system	Microsoft Windows 7 Professional (32bit) / Vista Business / XP Professional	
CPU	Intel® Celeron 420 (1.60 GHz or higher)	
	To use GFA-TV, Intel® Pentium DualCore E2180 (2 GHz) or higher is required.	
D 4 4 4	1 GB or higher (Vista) or 512 MB or higher (XP)	
RAM	To use GFA-TV, 1 GB or higher (GFA-TV)	
Monitor	XGA (1024 × 768 dots) or higher	
Storage device	One CD-ROM drive (for installing a software)	
Storage device	Requires 60 MB min. hard disk space for AA installation.	
	One serial port (for AA control)	
I/O port	USB 2.0 port (for GFA-TV)	
Peripheral device	Monitor, keyboard, mouse, printer	

* Notes

•The ASC-7000, ASK-7000 and GFA-7000A are optional accessories.

[·]The PC, monitor and printer are not included in the standard configuration. Prepare them separately.

[·]The separately available micro sampling kit is required for the flame micro sampling method.


Microsoft Windows 7 Professional / Vista Business and XP Professional are registered trademarks of Microsoft Corp., U.S.A.

[•]The AA-7000 Series does not conform to IEC60601 — Medical Electrical Equipment.



Installation Conditions


Dimensions

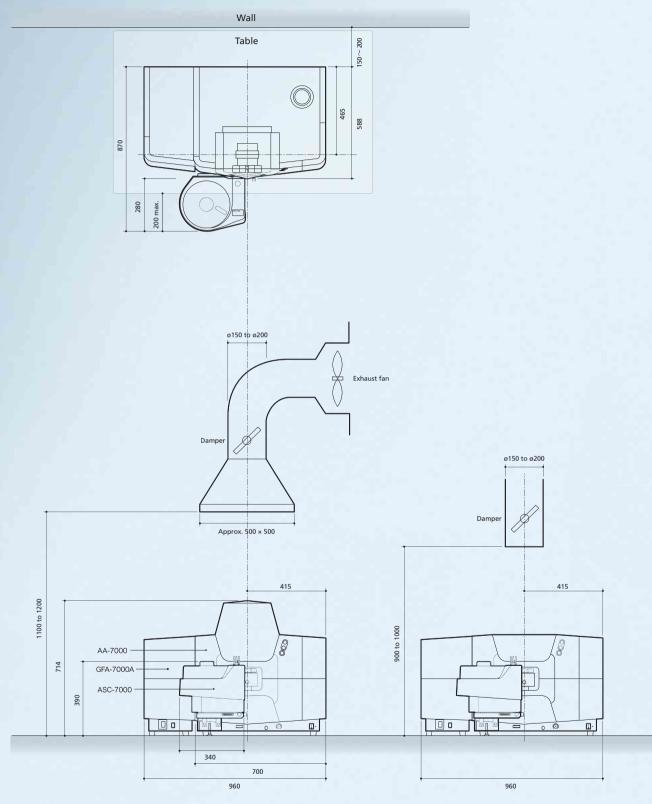


Both for flame analysis and furnace analysis

For furnace analysis

Make sure all required equipment is available before starting instrument installation. See the installation guidelines for details.



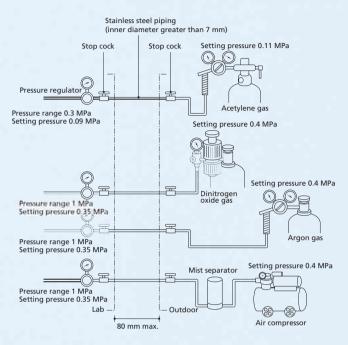

Operating	Temperature range	10 to 35 °C
environment	Humidity range	20 to 80% (less than 70% when temperature is higher than 30 $^\circ \text{C}$
		1500 mm min. (W) × 700 mm min. (D)
Testing bench		Withstand load: 200 kg *1, 2
Gas tube	Material	Stainless *3
Gas tube	Dimensions	7 mm min. I.D. × 80 mm min. (L)
	Acetylene	Cylinder: 0.11 MPa
		Lab: 0.09 MPa
Gas supply	Air	Compressor: 0.4 MPa
pressure		Lab: 0.35 MPa
(set secondary	Dinitrogen oxide	Cylinder: 0.4 MPa
pressure)		Lab: 0.35 MPa
	Argon	Cylinder: 0.4 MPa
		Lab: 0.35 MPa
	Material	Stainless
	Dimensions	For flame: Approx. 500 mm W × 500 mm D
Exhaust duct		For furnace: ø150 mm to ø200 mm
	Intelie conseitu	For flame: 600 to 1200 m³/hr
	Intake capacity	For furnace: 10 to 180 m³/hr
Cooling water (GFA-7000A)		Cooling water circulation unit or tap-water equipment *


*1 Atomic absorption spectrophotometer stand recommended

*2 Maintain a free maintenance space of 150 to 200 mm to the sides and rear of the instrument.
*3 Do not use pipes containing copper, silver, gold, mercury (or alloys containing these metals) as pipes for acetylene.

*4 If tap-water equipment is used, ensure that it meets the specifications below.

Compatible faucet	Faucet 13 or 12 to 15 mm O.D. rimmed faucet
Water temperature	10 to 30 °C
Water flow rate	0.6 to 1.5 L/min
Supply pressure	0.08 to 0.15 MPa *5
Supply port	7 mm min.

*5 If the supply pressure exceeds 0.17 MPa, use the optional Regulator ASSY.

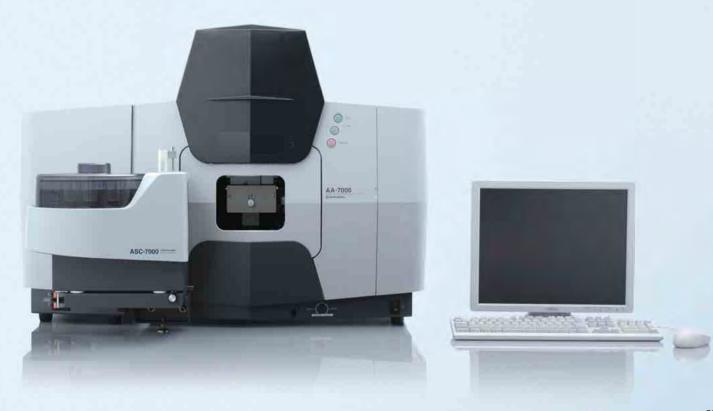



Shimadzu Corporation www.shimadzu.com/an/

Company names, product/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation or its affiliates, whether or not they are used with trademark symbol "TM" or "@". Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services. Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

For Research Use Only. Not for use in diagnostic procedures. The contents of this publication are provided to you "as is" without warranty of any kind, and are subject to change without notice. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication.

© Shimadzu Corporation, 2012 Printed in Japan 3655-05238-30ANS